
Chromatogram and Results

Injection Details

Injection Name:	**BLANK**	*Run Time (min):*	**12.00**
Vial Number:	**RA1**	*Injection Volume:*	**2.00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_2**
Calibration Level:		*Wavelength:*	**254**
Instrument Method:	**HPLC-02(LAB)**	*Bandwidth:*	**4**
Processing Method:	**HPLC-02(LAB)**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	################	*Sample Weight:*	**1.0000**

Chromatogram

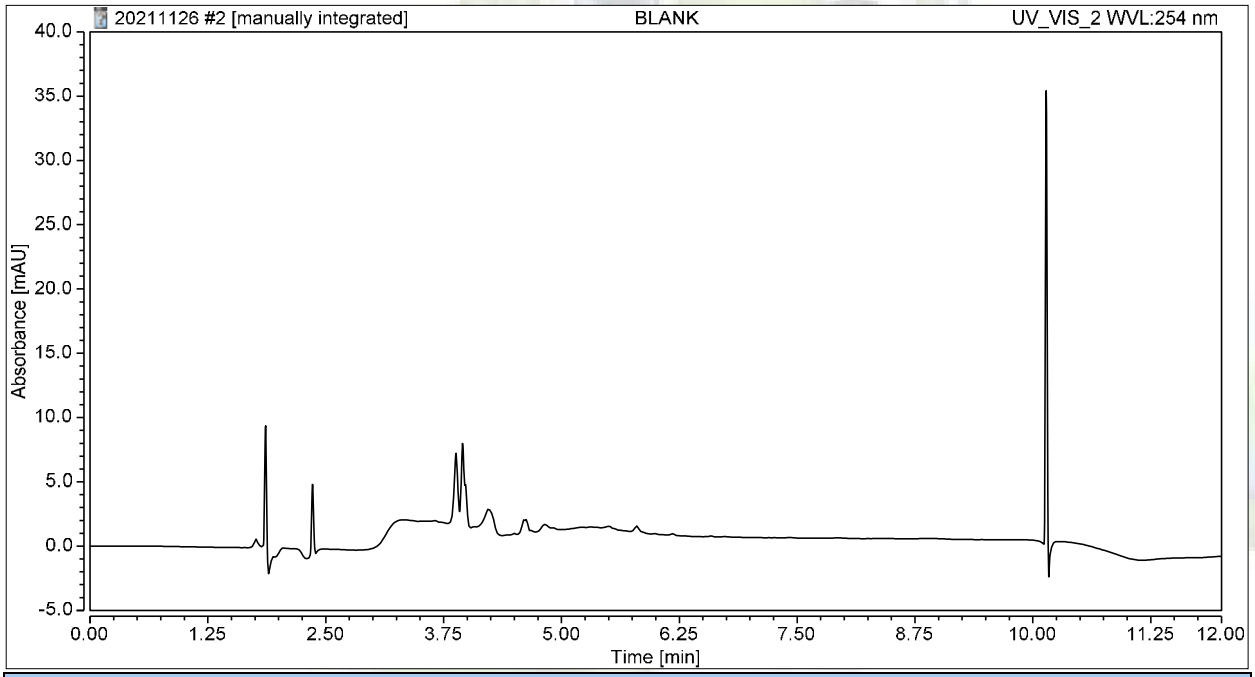

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount n.a.
Total:			**0.000**	**0.000**	**0.00**	**0.00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Chromatogram and Results

Injection Details

Injection Name:	**394-01-4**	*Run Time (min):*	**12.00**
Vial Number:	**BA2**	*Injection Volume:*	**1.00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_2**
Calibration Level:		*Wavelength:*	**254**
Instrument Method:	**HPLC-02(LAB)**	*Bandwidth:*	**4**
Processing Method:	**HPLC-02(LAB)**	*Dilution Factor:*	**1.0000**
Injection Date/Time:	################	*Sample Weight:*	**1.0000**

Chromatogram

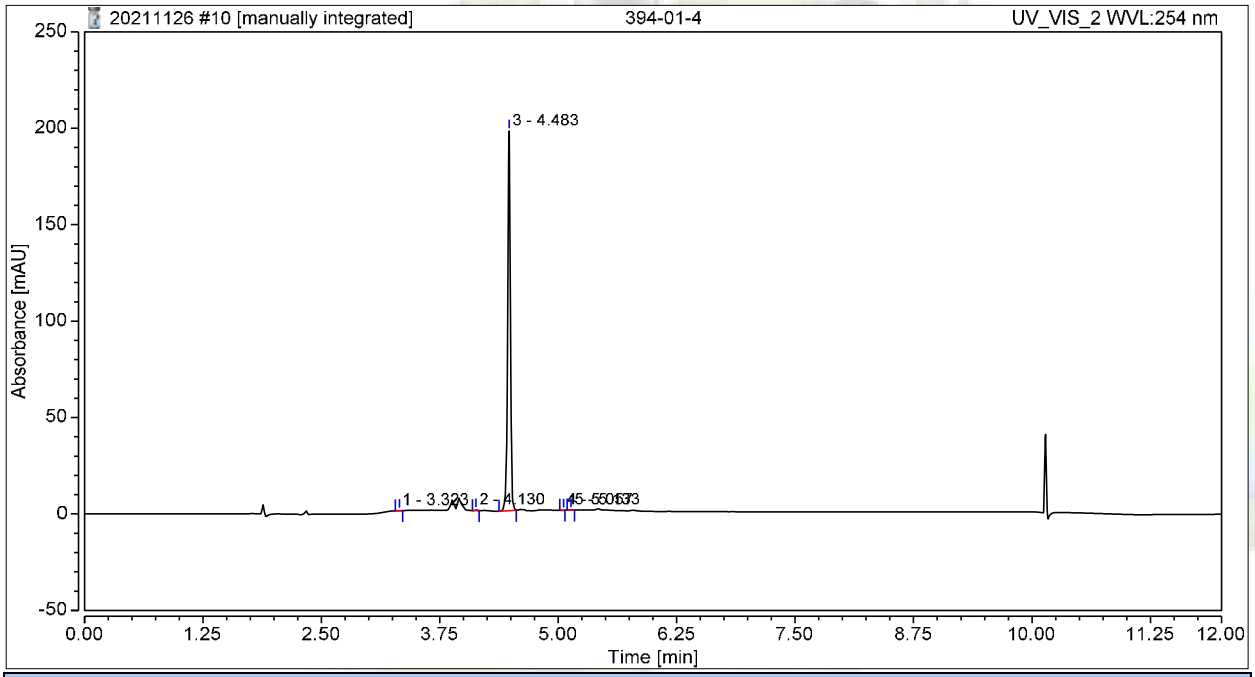

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount n.a.
1		3.323	0.004	0.084	0.06	0.04	n.a.
2		4.130	0.010	0.372	0.16	0.19	n.a.
3		4.483	6.544	196.785	99.74	99.73	n.a.
4		5.057	0.000	0.014	0.01	0.01	n.a.
5		5.133	0.002	0.063	0.03	0.03	n.a.
Total:			**6.561**	**197.319**	**100.00**	**100.00**	

Chromeleon (c) Dionex
Version 7.2.10.23925