




湖南沃凯生物科技有限公司
联系电话:13718666987 Tel:0744-2221508. Fax:0744-2221508
www.oka-vip.com M-ail:2577930172@qq.com

Data file: D:\CHEM32\1\DATA\220314\800055_22020033Final.D
Sample name: 800055_22020033Final
Description: Mobile phase: Buffer A: 0.1%TFA in H2O
Buffer B: 0.1%TFA in ACN
Gradient: 20-30% B in 20min, Flow rate: 1.0ml/min
Column: Unitary C18, 4.6*150mm, 5um 100A
Instrument: Agilent HPLC 1100
Instrument: 1100 Location: 84
Injection date: 2022/3/14 14:48:54 Injection: 1 of 1
Last changed: 2022/3/14 16:11:59 Injection volume: 10.000
Acq. operator: SYSTEM

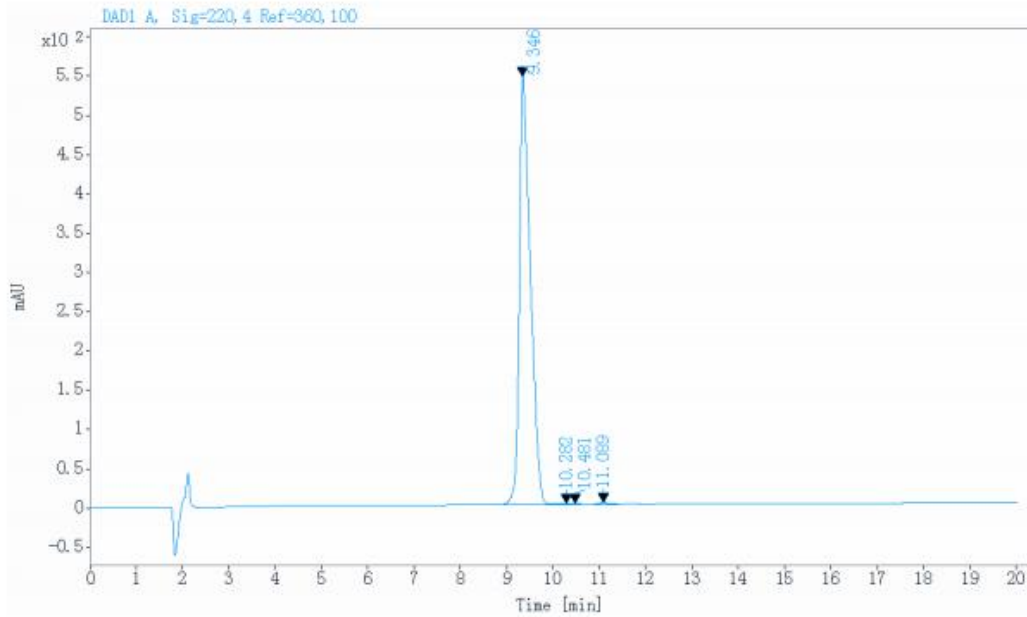

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT [min]	Type	Width [min]	Area	Height	Area%	Name
9.346	BV R	0.2382	8991.2666	545.8554	99.3009	
10.282	VV E	0.2775	27.6826	1.3485	0.3057	
10.481	VB E	0.1633	10.5760	0.9845	0.1168	
11.089	BB	0.2059	25.0426	1.8504	0.2766	
	Sum		9054.5679			