
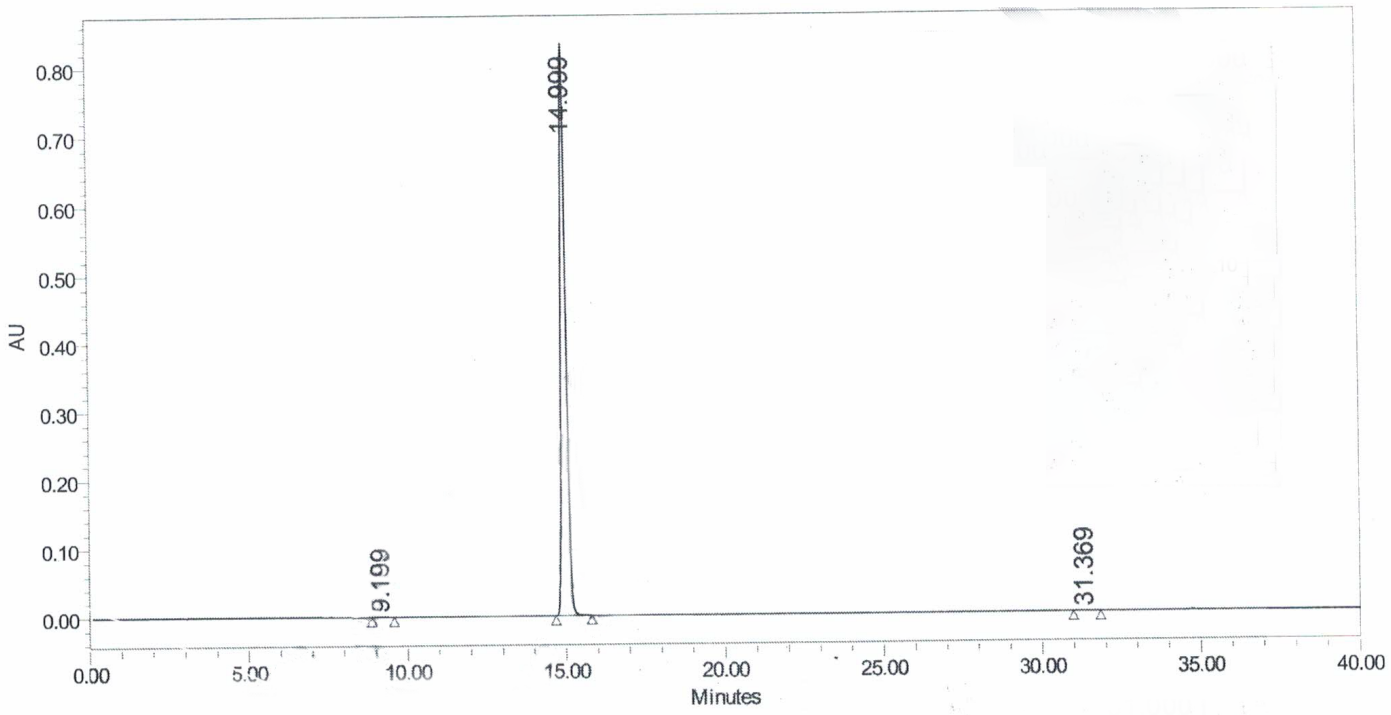


	RT	Area (μV*sec)	% Area	Height	Width (sec)
1	9.199	4263	0.05	269	42.000
2	14.999	9360058	99.89	832237	67.000
3	31.369	6232	0.07	247	51.000

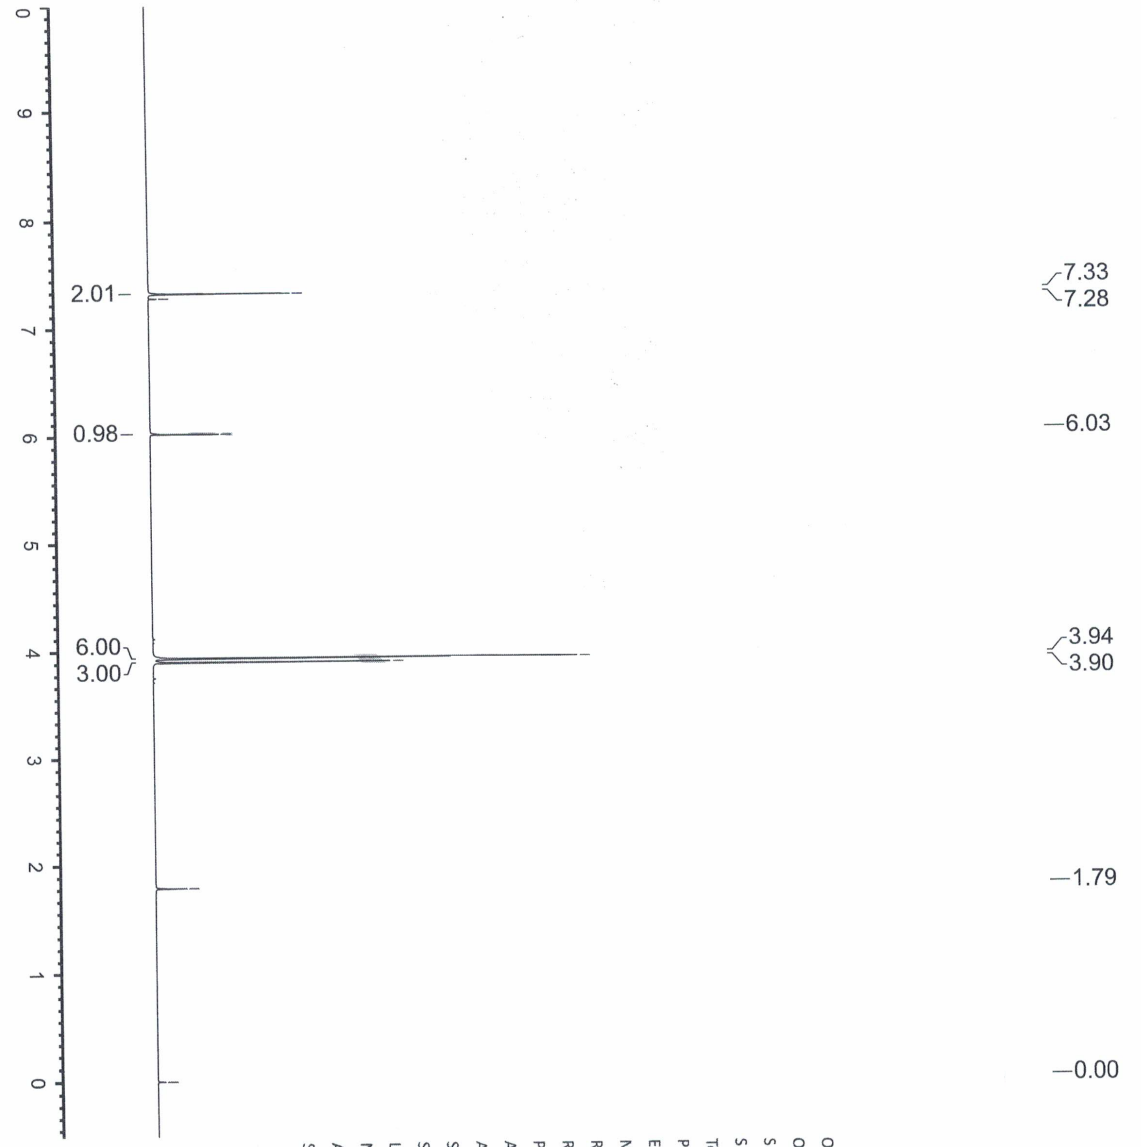

Parameter	Value
Origin	Bruker BioSpin GmbH
Owner	nmrsu
Spectrometer	spect
Solvent	CDCl3
Temperature	292.5
Pulse Sequence	zg30
Experiment	1D
Number of Scans	16
Receiver Gain	57
Relaxation Delay	1.0000
Pulse Width	9.7000
Acquisition Time	4.0894
Acquisition Date	2022-01-19T15:45:28
Spectrometer Frequency	400.13
Spectral Width	8012.8
Lowest Frequency	-1536.4
Nucleus	1H
Acquired Size	32768
Spectral Size	65536